

Network ID Camera

SP

Installation Instructions

NIC2-2 Quick Installation Guide

for MAMMOMAT 300/3000 or
compatible

© Siemens AG 2004

The reproduction, transmission or use of this document or its contents is not permitted without express written authority. Offenders will be liable for damages. All rights, including rights created by patent grant or registration of a utility model or design, are reserved.

Quick Installation Guide

For Siemens Mammomat 300/3000 or compatible



NIC2-2 Network ID Camera

General

This guide describes how to install and customize the Network ID Camera, herein called NIC, which has Siemens specified setup pre-installed, pre-configured.

Prerequisite

Verify that the following items are available/installed at the mammomat:

Siemens MAT-No.	Siemens VBLO-No.	Description
66 26 001	44 94 535	Printer connection kit
63 96 704	44 94 543	Isolation kit
65 61 521	44 94 568	"Triacon" Adapter cable

Unpacking

The box contains the NIC, a power cord, a converting cabel (to convert AUX1 from a RJ12 to a D-Sub 9 connector), an operator's manual and this document. The keyboard should be equipped with the country dependent keycaps.

Notice

Verify that the correct camera version was delivered concerning the used cassette type. A standard camera handle all known cassettes with standard C1 or C1N window except Fuji cassettes with telescopic lid. Two versions are currently available:

- Standard
- Fuji - Fuji cassettes with telescopic lid, for example type EC-AWU.

Installation



The Network ID Camera is classified as a Medical Device and fulfills EN 60950.

According to European Safety Regulations for Medical Equipments, the following conditions must be fulfilled:

- If the camera is operated within a distance of 1.5 m from the patient, it must be connected to the equipotential equalization device (E2D).

E2D with cable must be provided by the customer.

The purpose of the E2D is to ensure that all medical and other equipments are connected to the same ground potential. If, on installation, your Service Provider connected the camera to the equipotential bushbar using the equipotential bonding plug, this connection may not be interrupted, i.e. you are not allowed to pull off the cable coming from the equipotential bushbar (see illustration below).

- If the camera is connected to a Medical Equipment according to EN 60601-1(e.g. safety ground or data connections) the safety standard EN 60601-1-1 has to be met and documented.



E2D plug - Connector for the cable coming from the equipotential bushbar.

Place the unit on a steady shelf or table. If the camera is operated in a mobile unit, like mammography screening buses, it should be fastened to the surface with two screws mounted from the inside of the NIC.


The power cord should be connected to the power receptacle on the backside of the camera and to a wall outlet.




Power receptacle

! No voltage selection is necessary, the camera can be operated at any voltage between 100 - 250 VAC 50/60 Hz.

The communication cable should be connected to the AUX1 connector on the back of the camera and to the mammomat via the converting cable supply by Triacon.



AUX1 connector

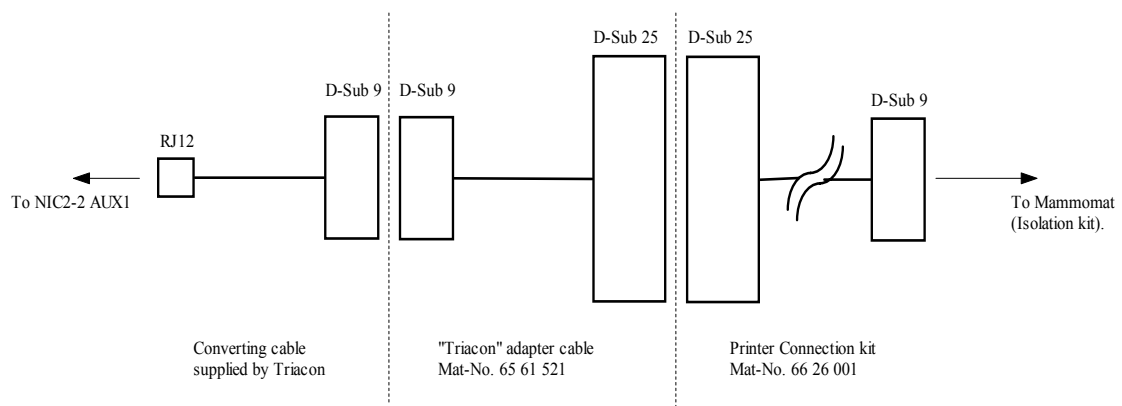

Setup

The NIC has a standard Siemens setup installed. The only thing to do is to change the hospital name, or delete it if not used. Also, if a Mammomat 300 is connected the communication protocol and active picture must be changed.

Enter Setup Mode

Enter Setup Mode by pressing SHIFT+F4 from main window.

```

Date: 26.06.2001      Time:13:37:48

Selected picture      : Mammo3000

Manual  Booking  Memory

```

Main window

After correct password has been given the setup window will appear.

```

Setup                               Ver: 2.2
Picture settings
Bookinglist configuration
Communication param
Settings
Sensor adjustment
Lock  Up  Down  Exit

```

Mammomat 3000

Enter 'Picture settings\Picture Mammo3000', move the highlight bar with up- and down arrow key, select by pressing ENTER. At position 23 of this field list one F-text field is present, this field is the hospital name.

No	Field	Length	Row,Col
19	Comm	4	28,198
20	F-text	19	28,228
21	H-line	19	38, 0
22	V-line	10	38,193
23	F-text	16	40, 0

Place New Remove Exit

To edit the field, just select it and press ENTER. Move the cursor with up-/down arrow keys to the 'Fixed text' field, edit the text.

```

Fielddefinition                     Field:23
Type: F-text
Row: 40      Column: 0
Fixed text:  General Hospital_      Font: Small
Save

```

When done press F4 key repeatedly until the main window appear.

Mammomat 300

1. Enter 'Communication param' and change the Protocol to "MMAT300". The 'Channel' should be "AUX1" (top right corner), if not press F1 ones. Move the cursor to the 'Protocol' with the arrow keys and select "MMAT300" with the F2- or F3 key.

```

Communication parameters Channel: AUX
Speed      9600
Parity     NONE
Databits   8 bits Protocol  MMAT300
Channel Previous Next Save

```

When done, press F4 ones to save and exit 'Communication parameters'.

- Enter 'Picture settings\Settings Mammo3000' and set 'Status' to "Not used". This will disable the Mammo3000 picture and automatically enable the Mammo300 picture.

Settings			
Status:	Used	Text:	Normal
Exposure:	100 ms	Location:	Bottom
Name: Mammo3000		Vert adjust:	16
		Def proj:	AP
		Previous Next Save	

When done, press F4 ones to save and exit 'Settings'.

- Enter 'Picture settings\Picture Mammo300', move the highlight bar with up- and down arrow key, select by pressing ENTER. At the bottom of the field list one F-text field is present, this field is the hospital name.

No	Field	Length	Row,Col
10:	Comm	6	28,204
11:	Comm	6	37,204
12:	H-line	19000	38, 0
13:	H-line	10	38,193
14:	F-text	16	40, 0
Place New Remove Exit			

- To edit this field, just select it and press ENTER. Move the cursor with up-/down arrow keys to the 'Fixed text' field, edit the text.

Fielddefinition		Field:23
Type:	F-text	
Row:	40	Column: 0
Fixed text:	General Hospital_	Font: Small
		Save

When done, press F4 repeatedly until the main window appear.

Set Time and Date

To set the clock, press SHIFT+F1 from the main window.

Change date and time	
19-02-01	15:56:17
Increase Decrease Save	

Use left- and right arrow keys to select a value and adjust it by pressing F2 or F3 key.

When done, press the F4 key.

Set Top or Bottom marking

Standard setting for the location of the marking on the film is bottom. To change this setting, enter 'Picture settings\Settings Mammo3000 or Settings Mammo300' and set 'Location' to "Top" and 'Vert adjust' to "0". This will set the marking to the top of the film. For bottom marking, set 'Location' to "Bottom" and 'Vert adjust' to "16"..


Settings			
Status:	Used	Text:	Normal
Exposure:	100 ms	Location:	Bottom
Name: Mammo3000		Vert adjust:	16
		Def proj:	AP
		Previous Next Save	

Installation Test

After installation the physical connection and settings in NIC must be verified. To do so, open the patient data window by pressing the F1 key from the main window and send data from the Mammomat. If all works as expected a number of values, such as kV, mAs etc., should appear on the display. If no data appear on the display, please refer to section 'Trouble shooting'.

Now, enter patient data into the Birthdata and Name fields. Mark a film and develop it. If the marking is too dark or light use one of the following two methods to correct this.

1. For fine tune use the operator accessible exposure settings window. This window is accessed from the patient data window by pressing SHIFT+F4.

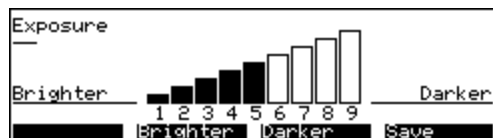

A higher value means longer exposure time according to the following:

1	2	3	4	5	6	7	8	9
0,5	0,6	0,71	0,84	1	1,19	1,44	1,68	2

The actual exposure time is the basic exposure time multiplied by a factor. Factory default 5 (factor = 1). The basic exposure time is set under 'Setup\Picture settings\Settings', please refer to method two below.

Note that this adjustment is intended for the user to fine tune the density of the marking. If a high (8 or 9) or low (1 or 2) value is required it is recommended that method number two is used.

2. Under 'Setup\Picture settings\Settings' the basic exposure time can be adjusted.

The exposure time can be a value between 10 and 65535. Default value is 100ms.

Communication problems

If no data is received from the Mammomat (i.e. no data is displayed on the NIC) a built in serial analyzer can be used to determine whether any data is received or not. This analyzer is connected to the HOST communication port which means that the communication cable from the Mammomat must be moved to this connector.



HOST connector

Enter Setup\Serial analyzer.

Serial analyzer																
-40:	00	00	00	00	00	00	00	00	00	00	00	00	00	00	00	00
-32:	00	00	00	00	00	00	00	00	00	00	00	00	00	00	00	00
-24:	00	00	00	00	00	00	00	00	00	00	00	00	00	00	00	00
-8:	00	00	00	00	00	00	00	00	00	00	00	00	00	00	00	00
0:	00	00	00	00	00	00	00	00	00	00	00	00	00	00	00	00
Refresh Exit																

The analyzer is displaying all data received in HEX and in plain text using ISO 8859-1 character set.

The soft-keys are used as follow:

- Refresh, press F1 to update the window.
- Exit, press F4 to exit the analyzer
- Clear Buf, press SHIFT+F1 to erase all data in the analyzer.

! Remember to move the communication cable back to the AUX1 connector after your test.